

Fig. 4



Fig. 5

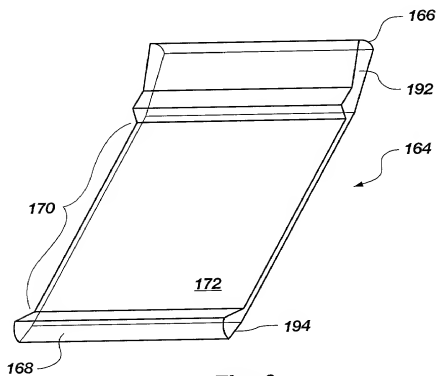


Fig. 6

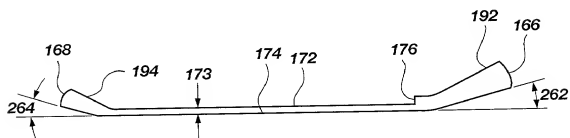


Fig. 7

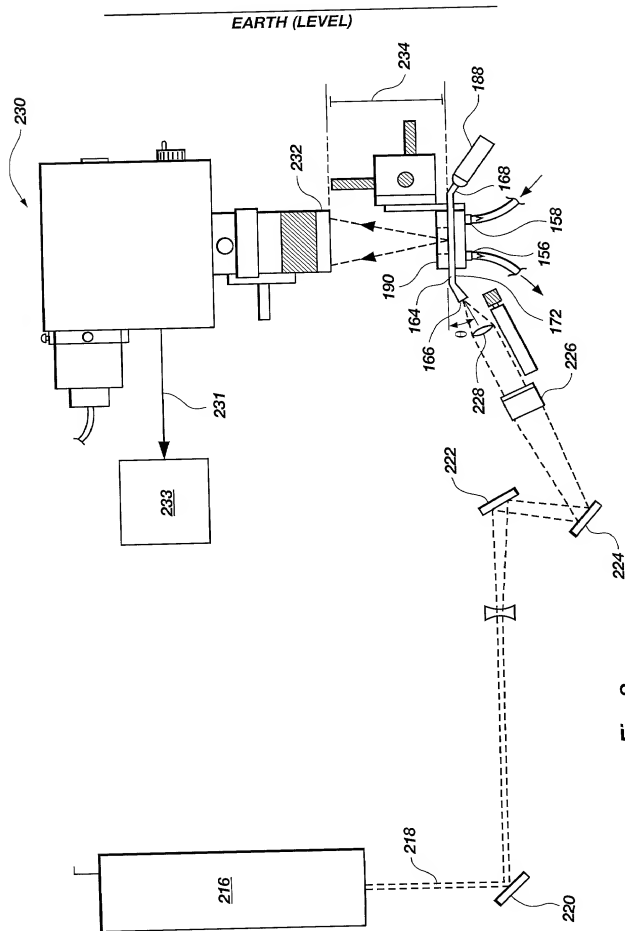


Fig. 8

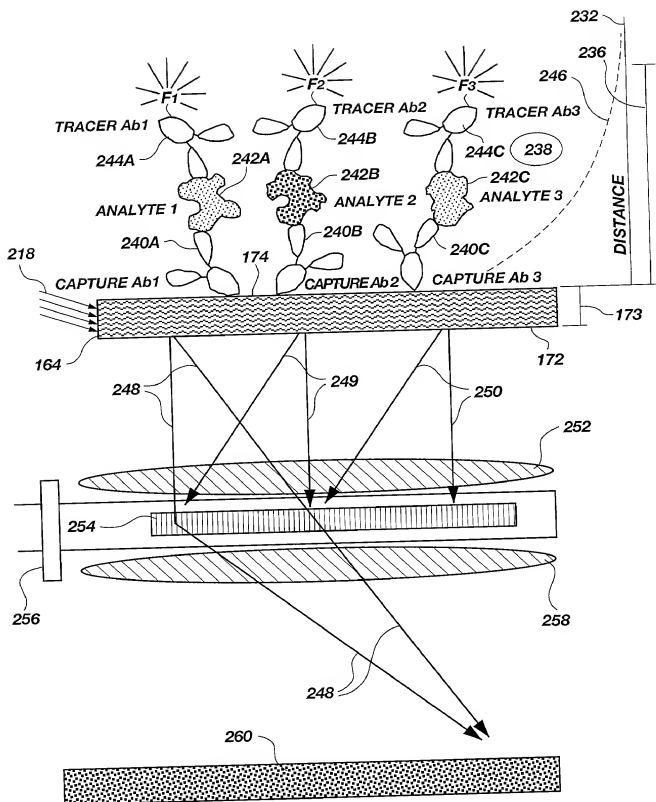


Fig. 9

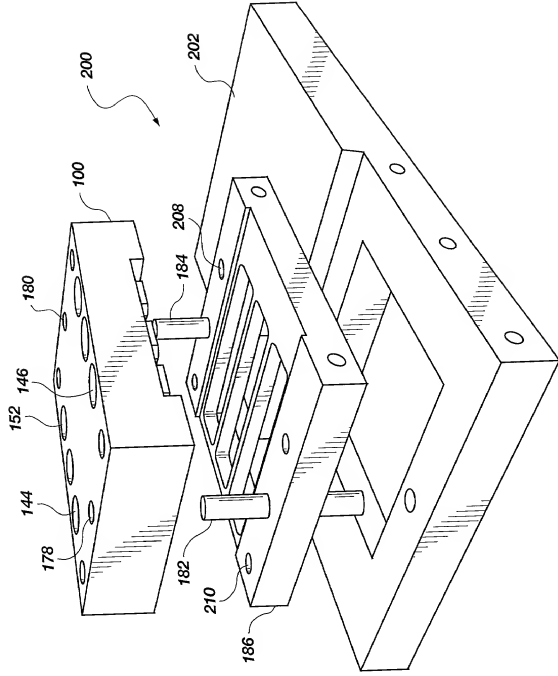


Fig. 10

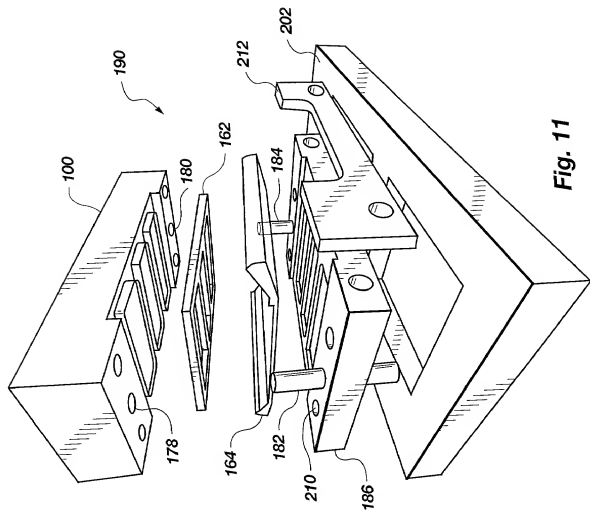


Fig. 11

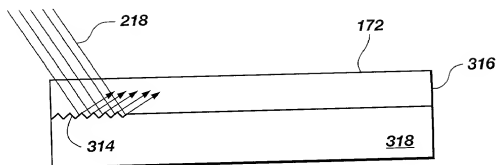


Fig. 12

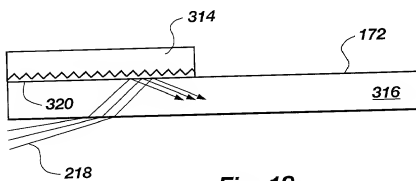


Fig. 13

Channel 1 Relative Errors (%) of Slope Parameter in the Linear Curve Fit of Myoglobin Assay Data

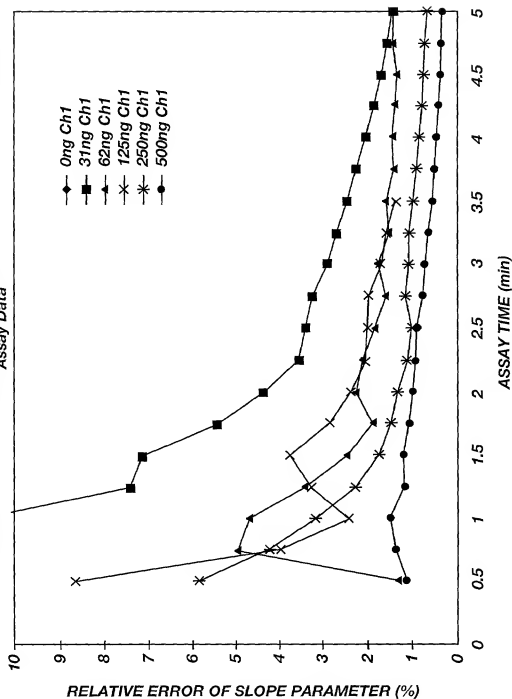


Fig. 14

100240-54262600

Channel 1 Myoglobin Assay Standard Curve (Using Linear Regression) at
Various Assay Times

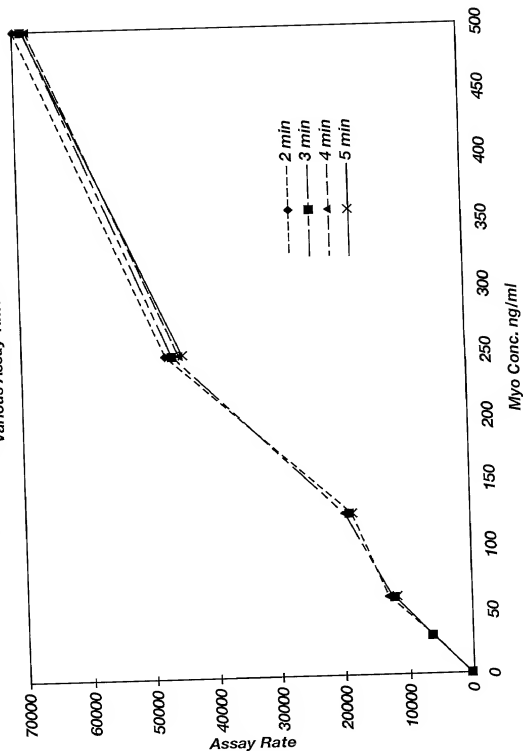


Fig. 15

442910-2405860






Fig. 16

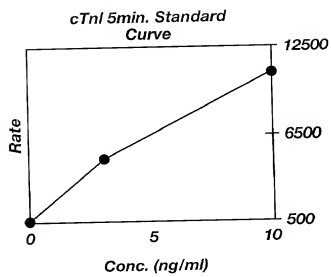


Fig. 17






Fig. 18

00240" B 2405800

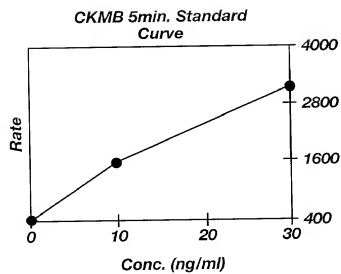


Fig. 19






Fig. 20

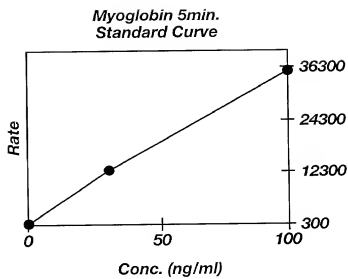


Fig. 21